




StableFlight Heli-Bag Complete Operational Package

Part Number: CRC-HRB-SFCOP

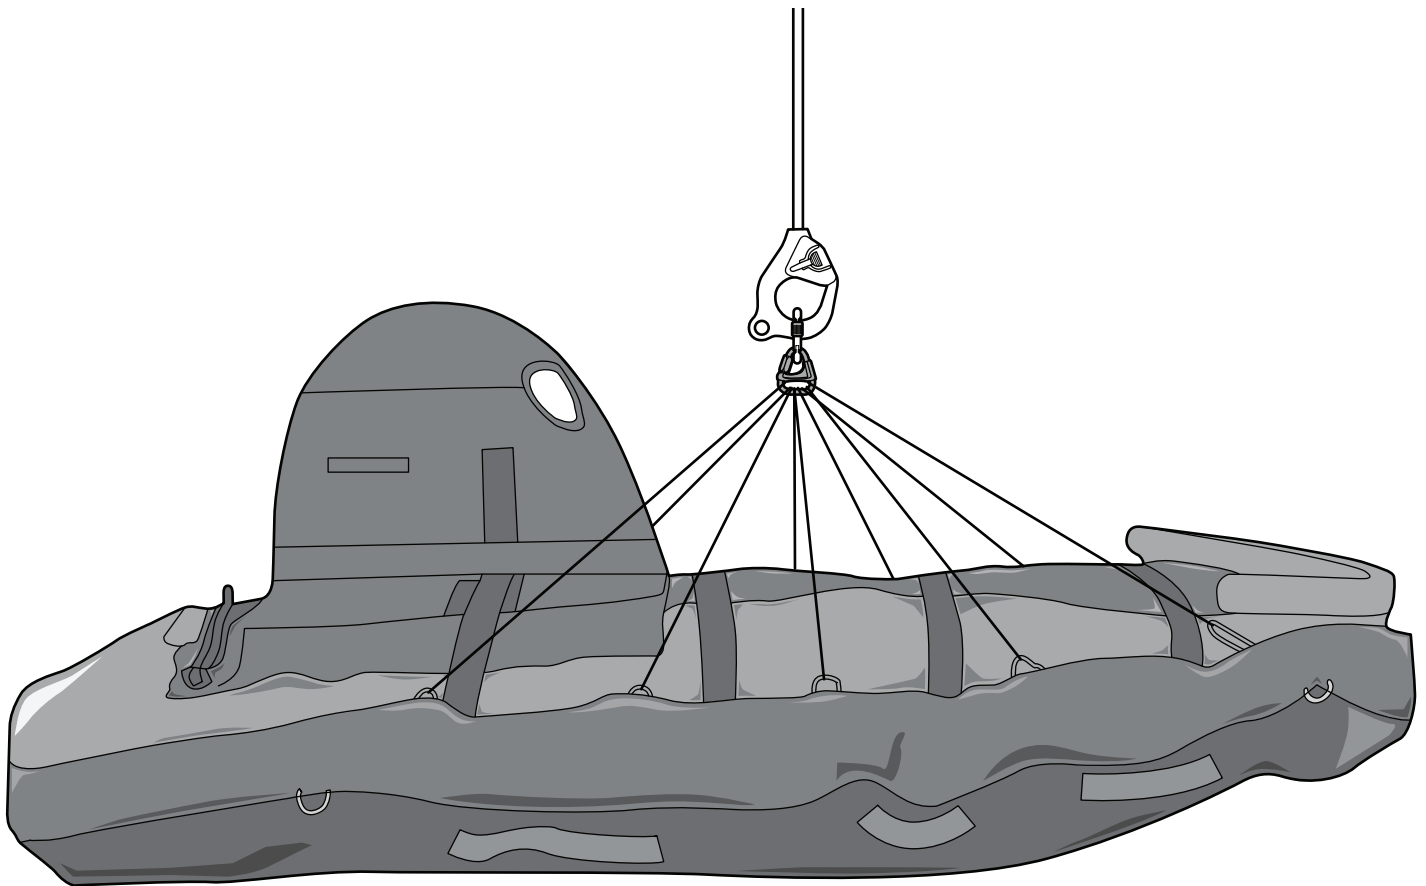

PLEASE SAVE THESE INSTRUCTIONS

TABLE OF CONTENTS

DIAGRAMS, DIAGRAMAS, SCHÉMAS.....	1
MANUAL TEXT	12
1. Safety Information	12
2. Use of This Manual.....	12
3. Field of Application	12
4. Key	12
5. Specifications	12
6. Certifications.....	12
7. Nomenclature.....	13
8. Inspection/Removal from Service	13
9. Instructions for Use.....	13
10. Limitations	14
11. Care and Maintenance	14
12. Compatibility	14
13. Lifespan	14
14. Warranty	14
15. Equipment Record.....	14
16. Training Record	14
TEXTO DEL MANUAL	14
TEXTE DE LA NOTICE.....	17

DIAGRAMS

4. Key



PROPER USE
USO CORRETTO
UTILISATION CONFORME



USE WITH CAUTION
USAR CON PRECAUCIÓN
À UTILISER AVEC PRÉCAUTION



PROHIBITED USE
USO PROHIBIDO
UTILISATION NON AUTORISÉE

7. Nomenclature

(A)




(B)

(C)


(D)

(E)


(F)

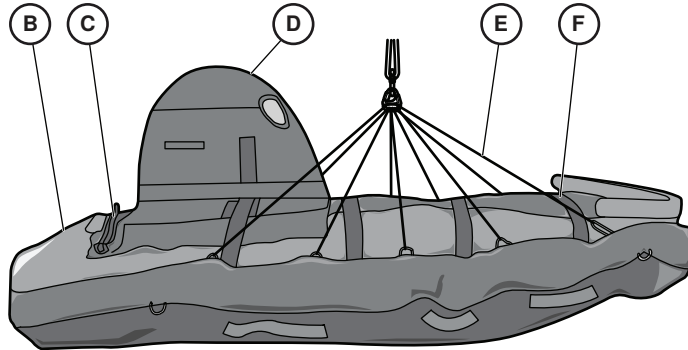


(G)

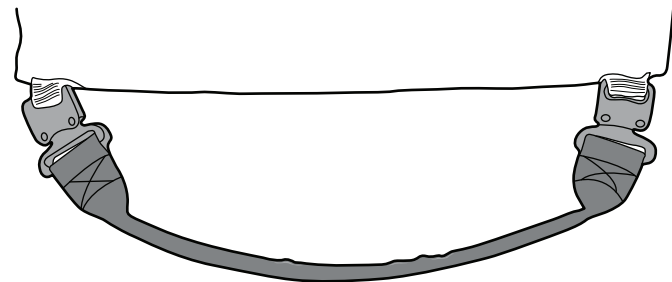


(H)

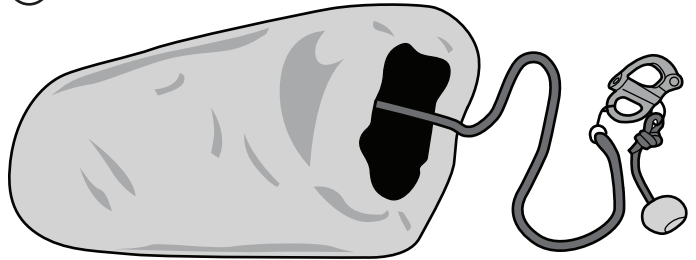


(J)

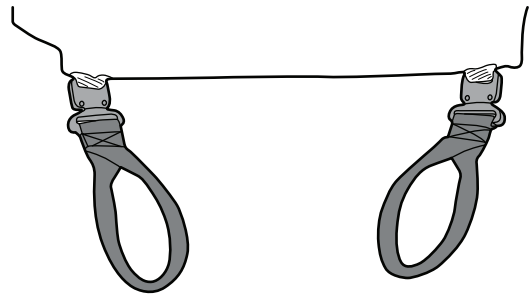








(K)

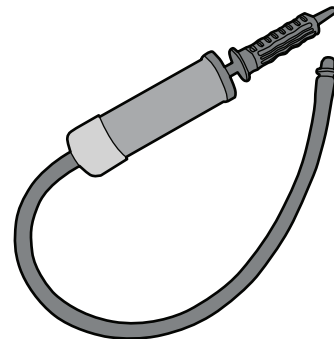


(L)

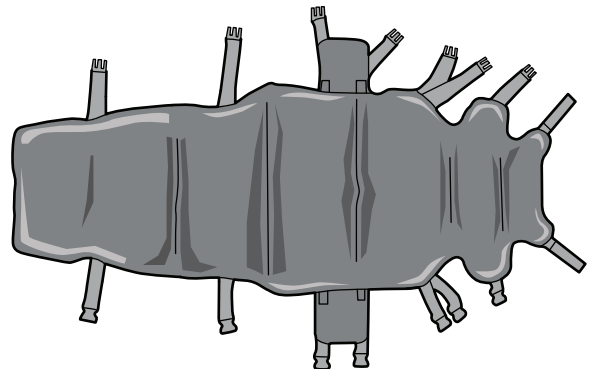




8. Inspection/Removal From Service

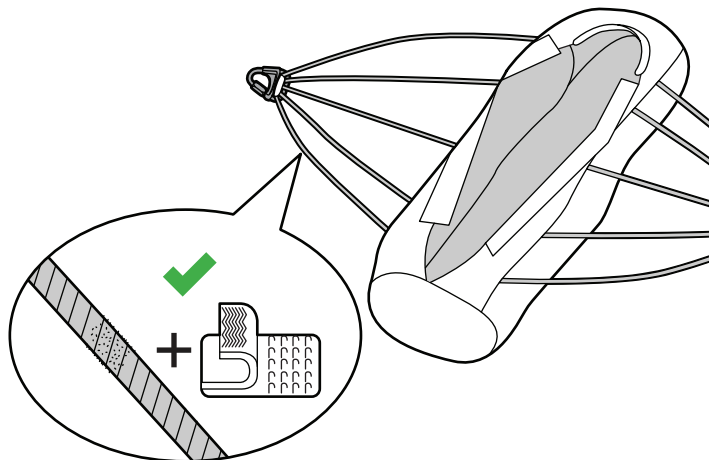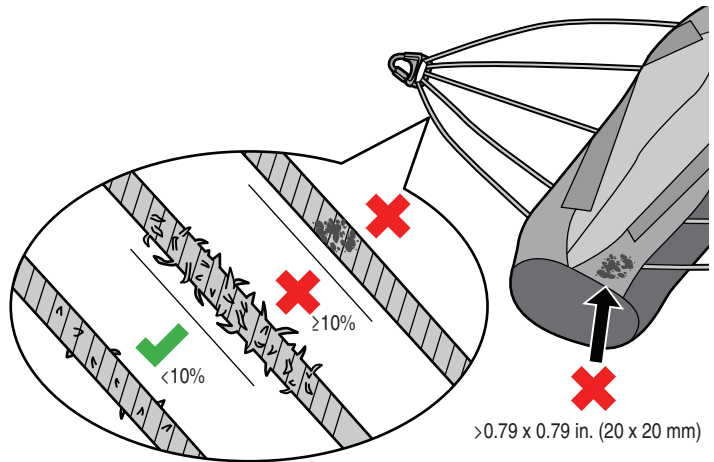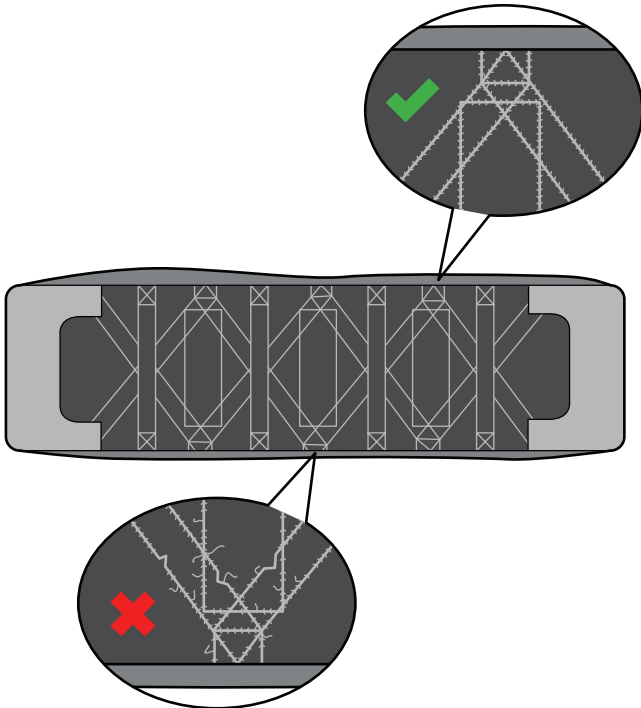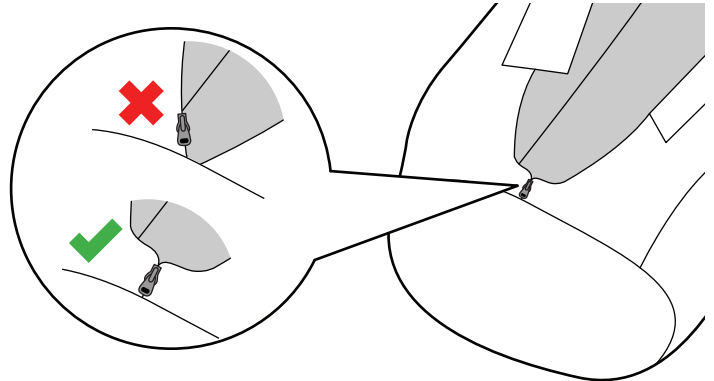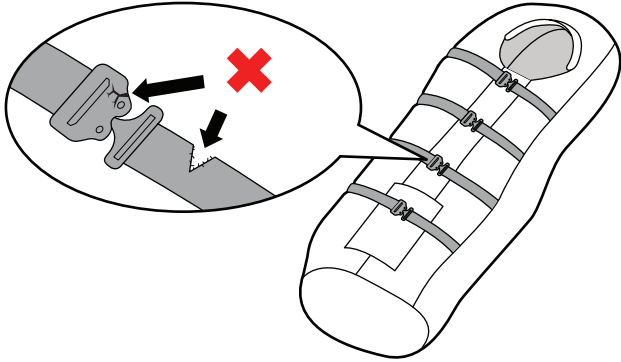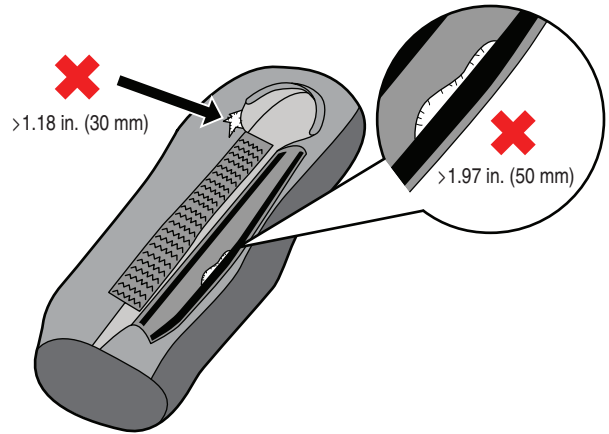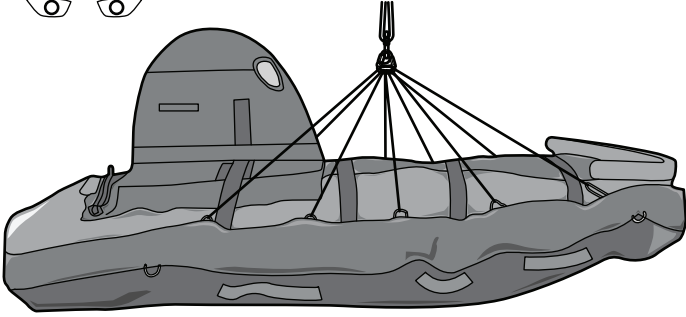




8. Inspection/Removal From Service (Continued)

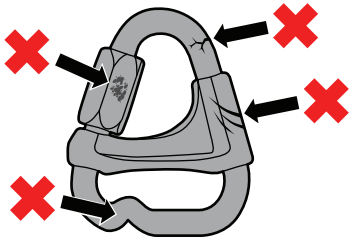


9.1. Pre-use Inspection

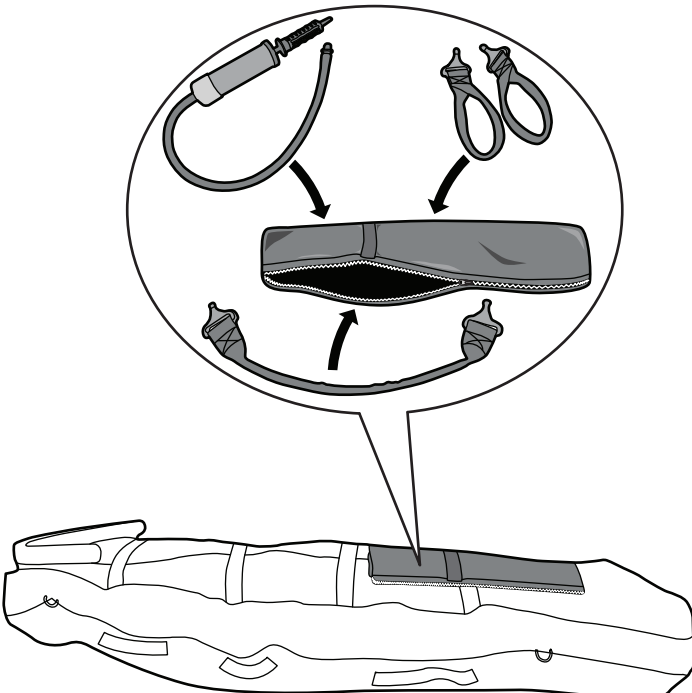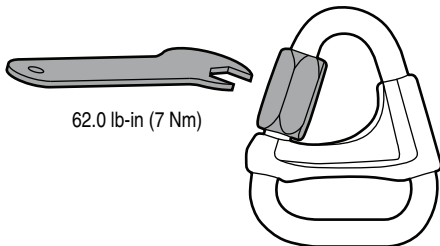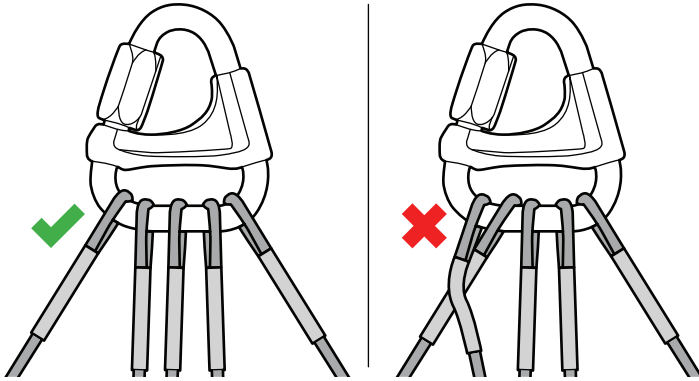






9.1.1. Installation of the Rotational Braking System (RBS)

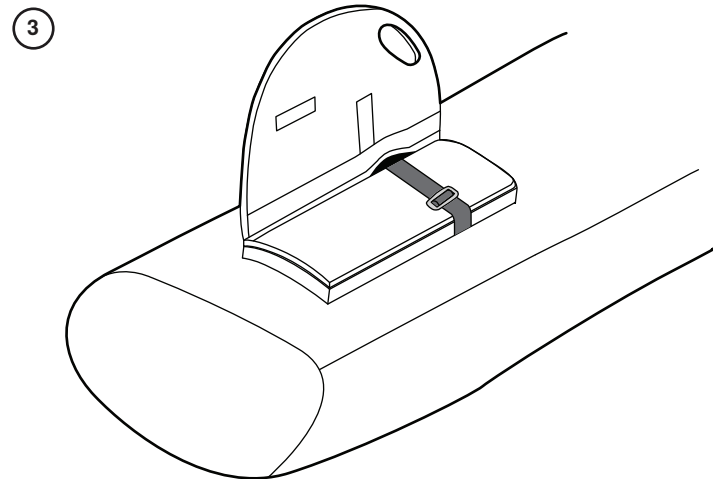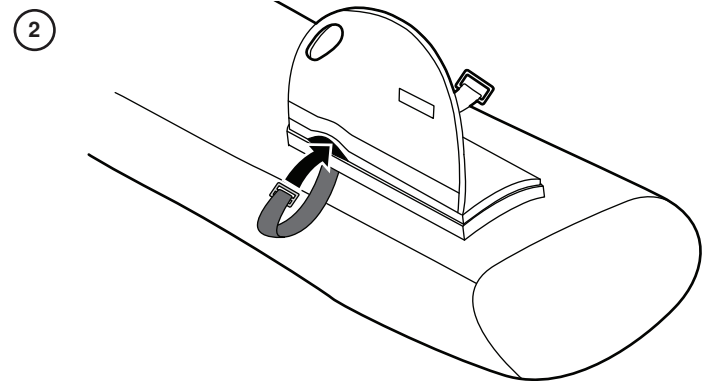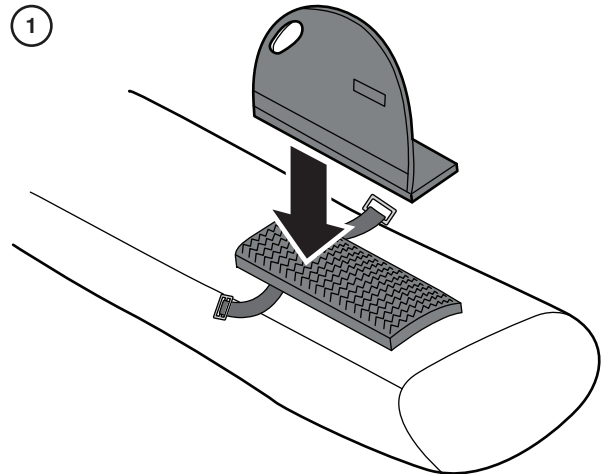

9.2. Preparation of the StableFlight Heli-Bag

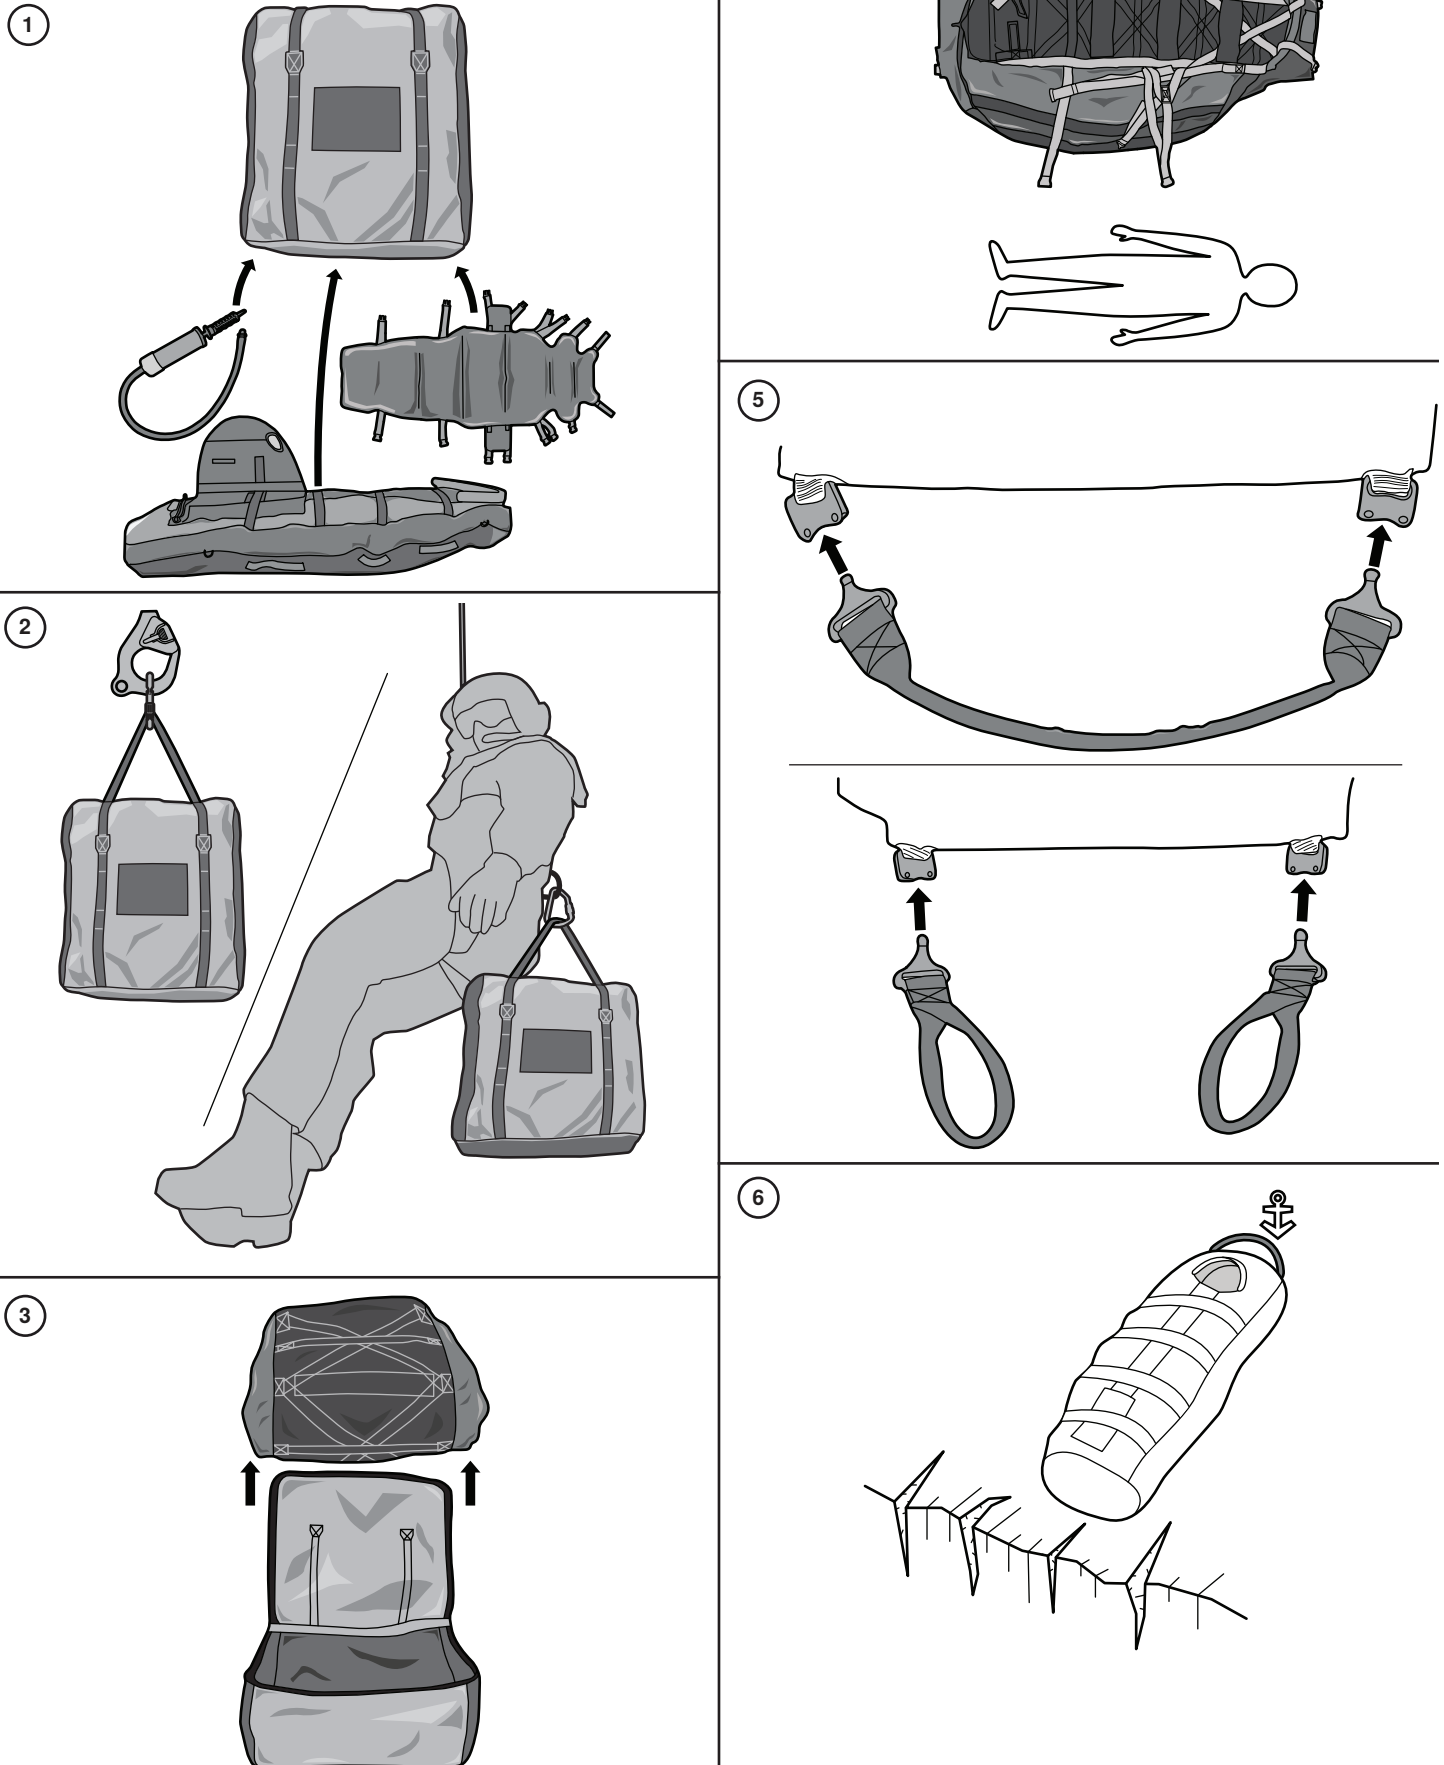

9.3.1. Option 1: Packaging the Patient Using Spinal Stabilization Inside the StableFlight Heli-bag

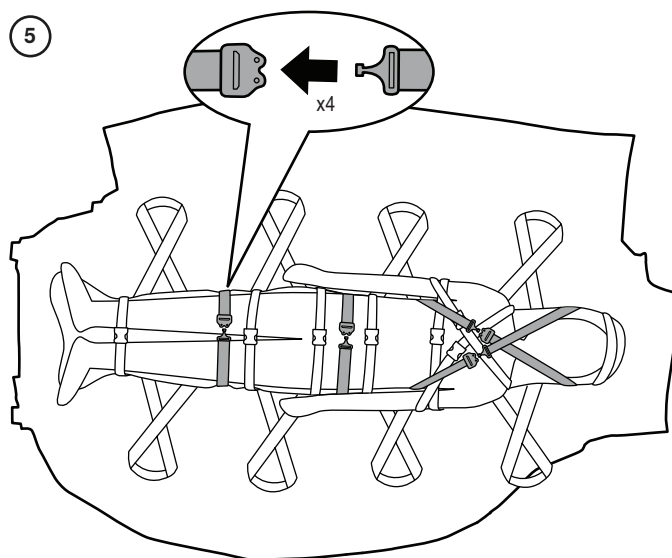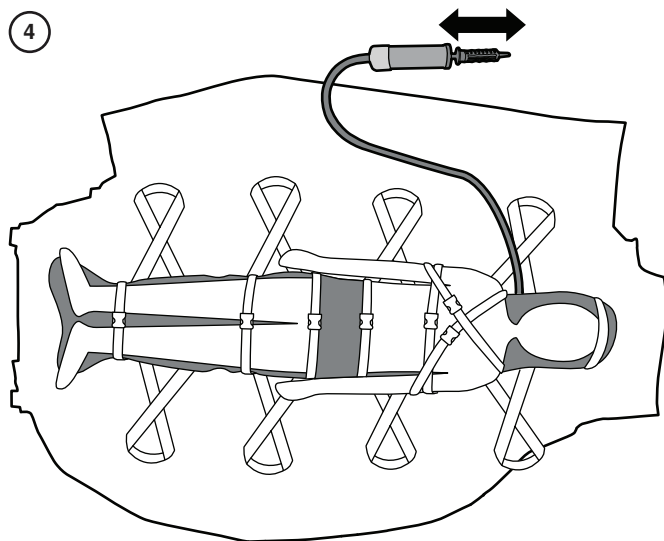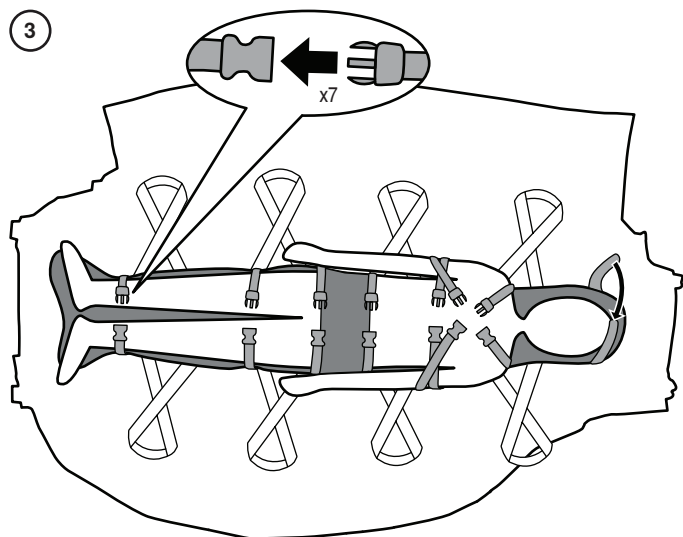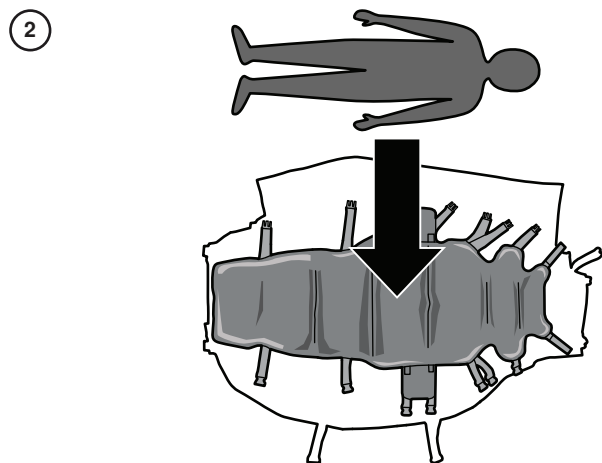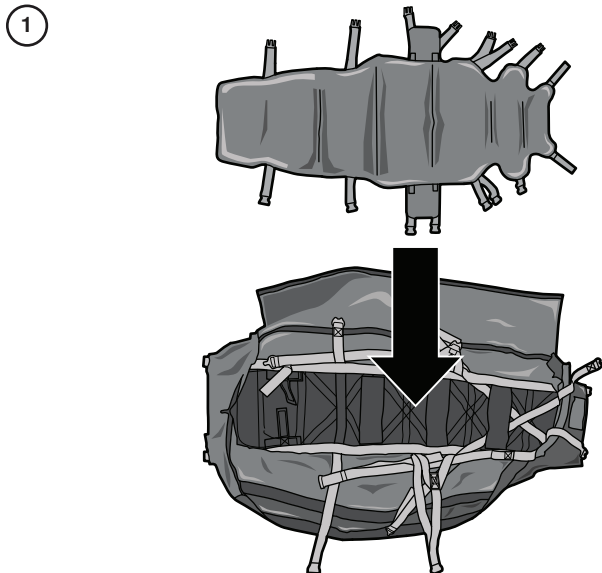


Proceed to DIAGRAMS section 9.3.4 for final steps.

Continúe con la sección 9.3.4 de DIAGRAMAS para conocer los pasos finales.


Passez à la section DIAGRAMMES 9.3.4 pour les dernières étapes.

9.3.2. Option 2: Packaging the Patient Using Spinal Stabilization Outside the StableFlight Heli-bag


1

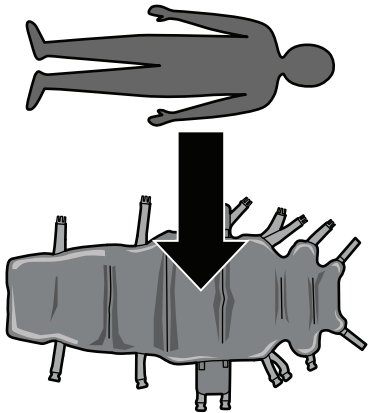


2

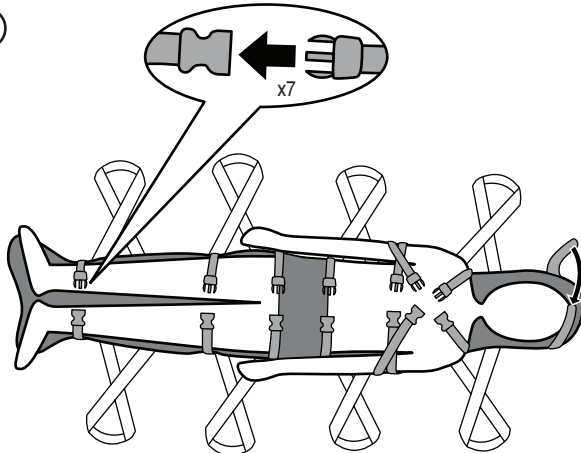


3

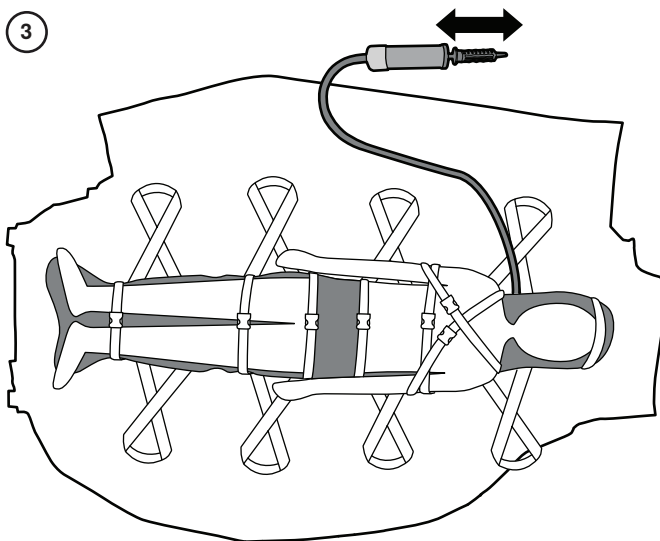

4

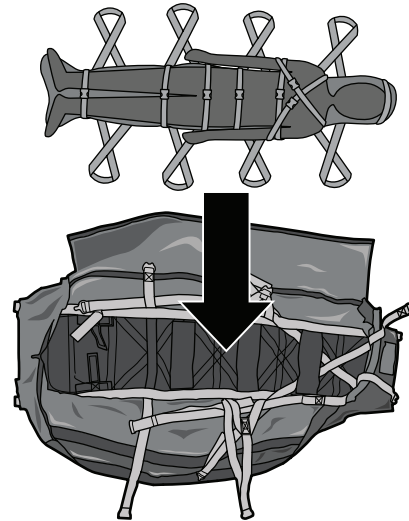

5

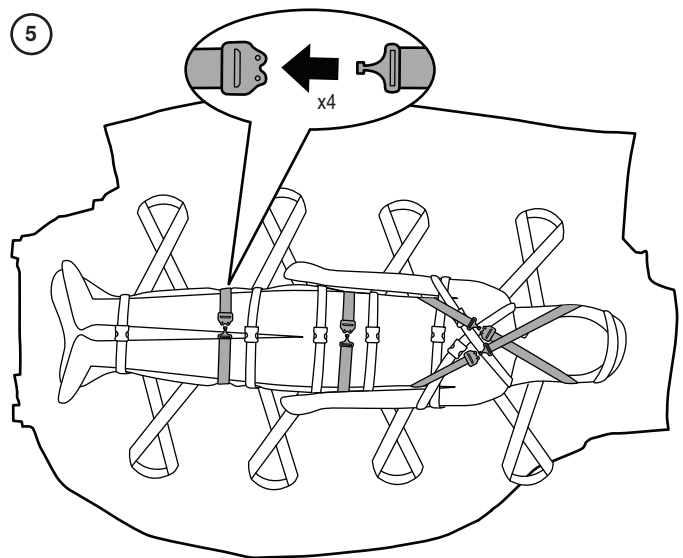



Proceed to DIAGRAMS section 9.3.4 for final steps.

Continúe con la sección 9.3.4 de DIAGRAMAS para conocer los pasos finales.



Passez à la section DIAGRAMMES 9.3.4 pour les dernières étapes.

9.3.3. Option 3: Packaging the Patient Using a Litter

1

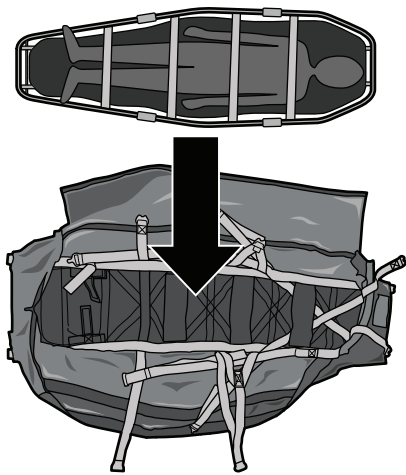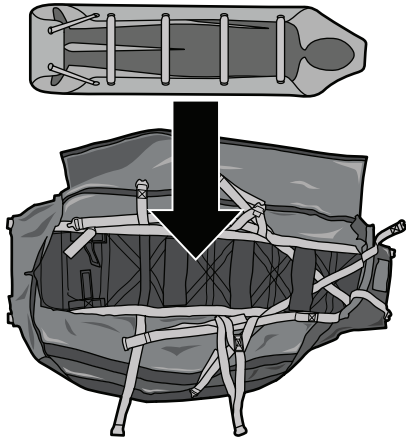

2

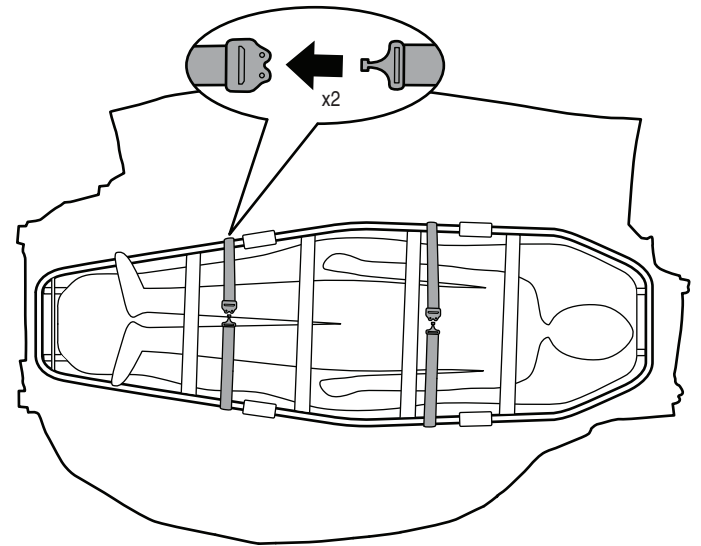
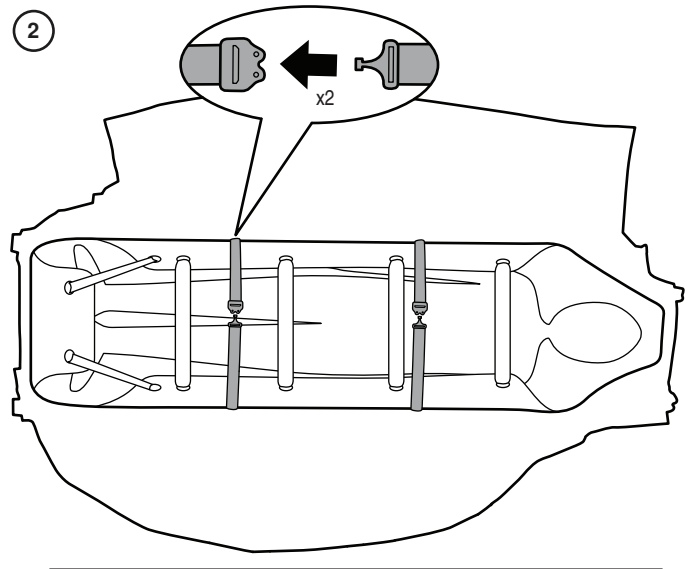


Proceed to DIAGRAMS section 9.3.4 for final steps.




Continúe con la sección 9.3.4 de DIAGRAMAS para conocer los pasos finales.

Passez à la section DIAGRAMMES 9.3.4 pour les dernières étapes.


9.3.4. Final Steps Before Transport

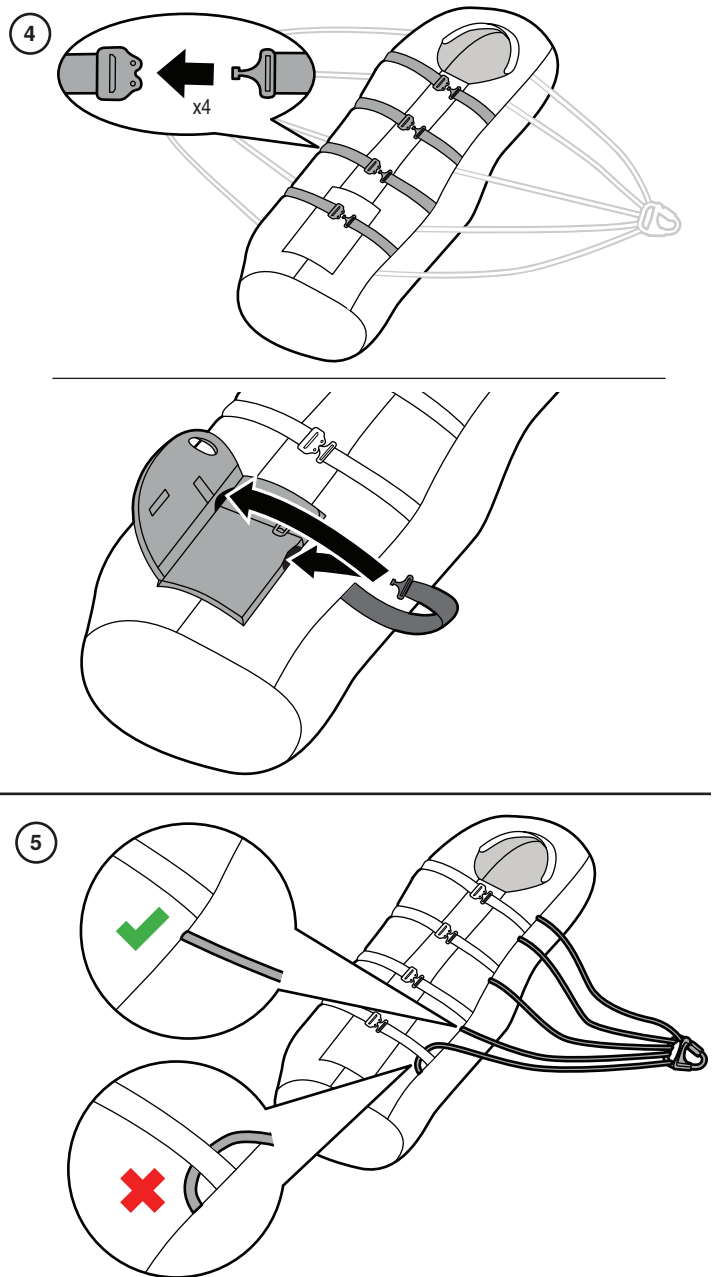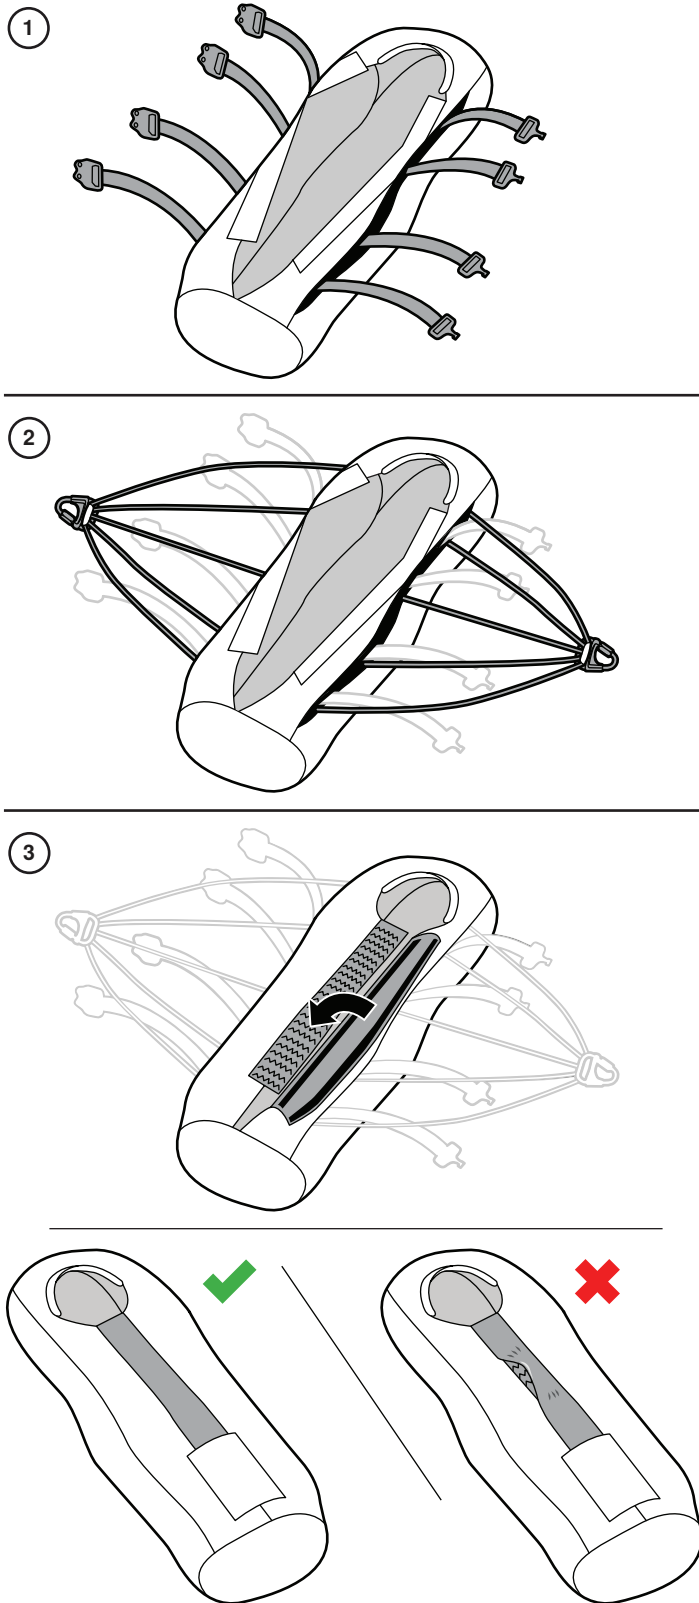

11. Care and Maintenance

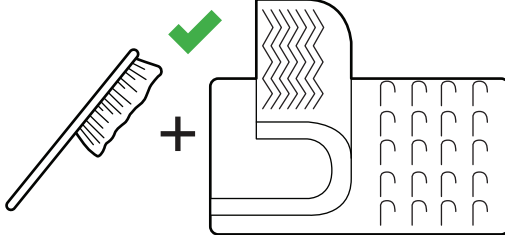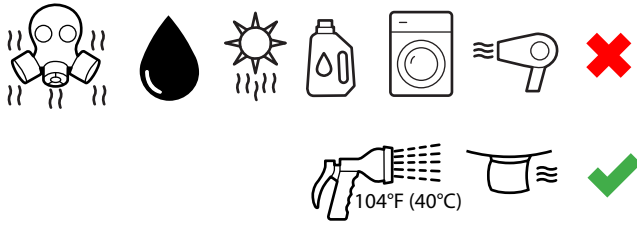


12. Compatibility

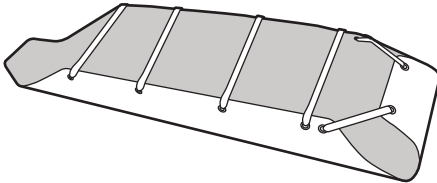

PE



+

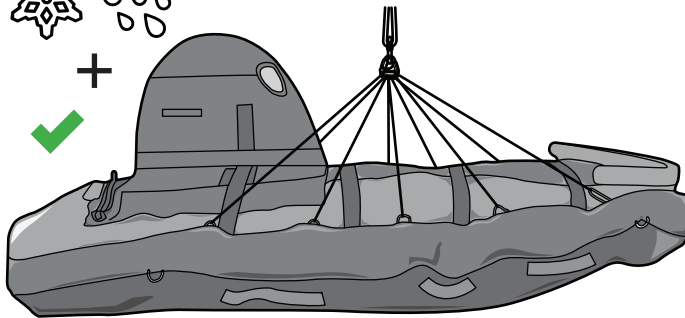

15. Equipment Record

Year of manufacture:		Purchase date:		Date first put into use:	
Año de fabricación:		Fecha de compra:		Fecha del primer uso:	
Année de fabrication :		Date d'achat :		Date de première utilisation :	
Other important information (i.e. document number):					
Otros datos importantes (por ejemplo, número de documento):					
Autre information importante (numéro de document) :					

[illegible]

16. Training Record

[illegible]



Country of Manufacture - USA

Cascade Rescue Company

1808 Industrial Drive, Sandpoint, ID 83864 USA
Telephone: +1 208-263-2484 • Toll Free +1 844 414-RESQ
Web: www.cascade-rescue.com • Email: SRsupport2@harken.com

Manufacturer - Harken, Inc.

N15W24983 Bluemound Rd., Pewaukee, WI 53072-4974 USA
Telephone: +1 262 691-3320
Web: www.harken.com • Email: SRsupport2@harken.com